


# Arrow® Short-term Peripheral Access Device Selection Tool

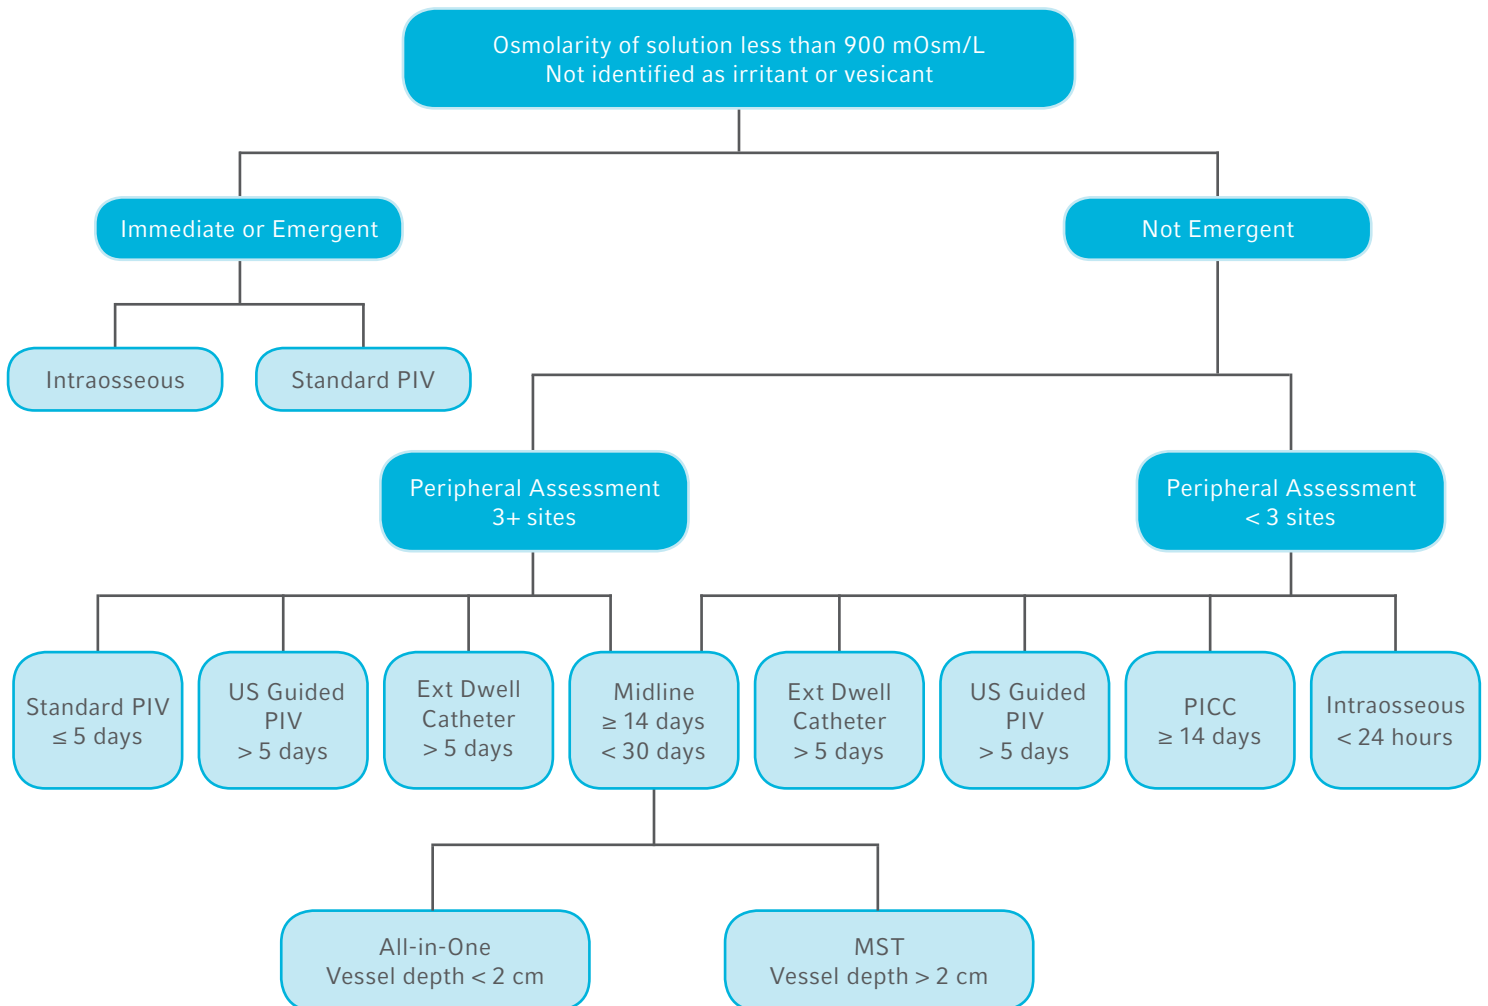

*Device selection tools should be used in combination with individual patient assessment as a general guideline. Clinical practice may vary based on institutional policy and patient needs.*

References:

1. Gorski LA, Hadaway L, M.Hagle, McGoldrick M, M.Orr, Doellman D. 2016 Infusion therapy standards of practice. *Journal of Infusion Nursing*. 2016;39(1 Suppl):S1-S159.
2. Chopra, V et al. The Michigan Appropriateness Guide for Intravenous Catheters (MAGIC): Results From a Multispecialty Panel Using the RAND/UCLA Appropriateness Method. *Ann Intern Med*. 2015;163:S1-S39. doi:10.7326/M15-0744

Rx only

Teleflex, the Teleflex logo, and Arrow are trademarks or registered trademarks of Teleflex Incorporated or its affiliates, in the U.S. and/or other countries.

Information in this material is not a substitute for the product Instructions for Use.

© 2018 Teleflex Incorporated. All rights reserved. MC-004111 Rev 0.1